




PH-5 CT Abdomen Phantom

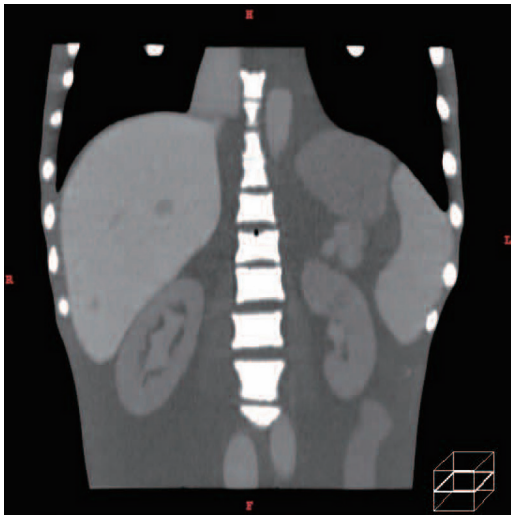


coronal

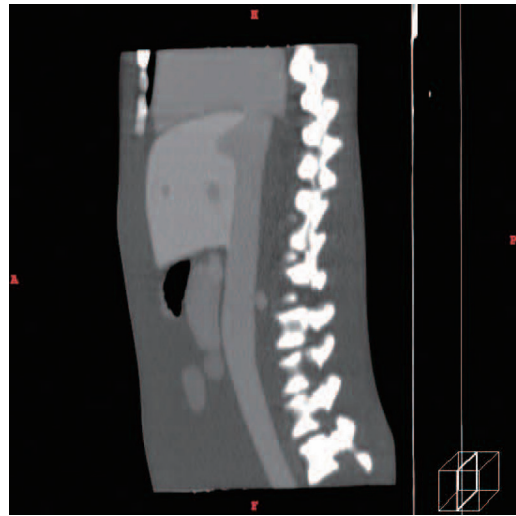

sagittal

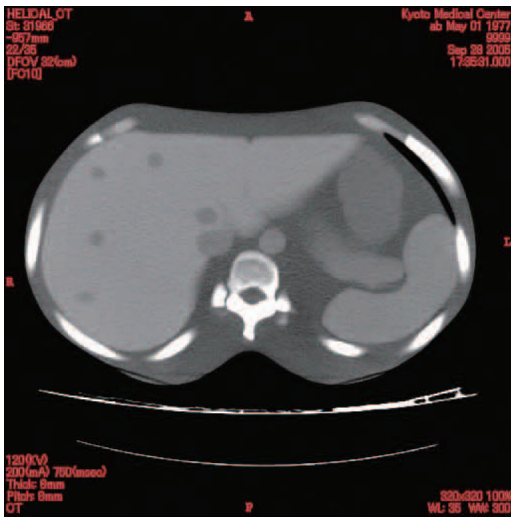


axial

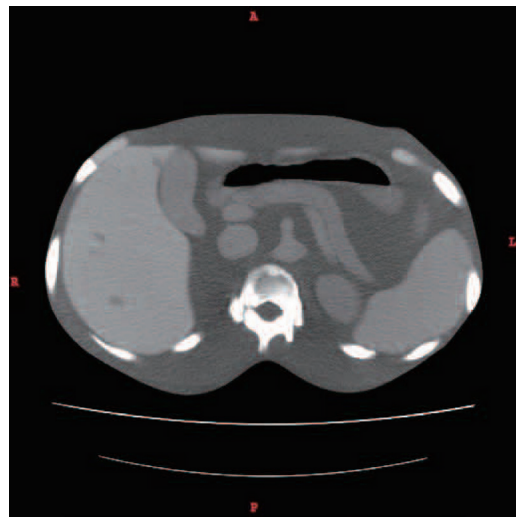

80kV



110kV

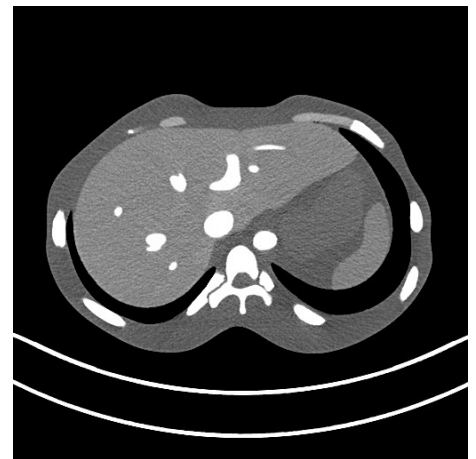

130kV



Specifications are subject to change without our prior notice.

For the latest information and further details, check our website www.kyotokagaku.com,

follow us on **Facebook** www.facebook.com/kyotokagaku or **contact us at** rw-kyoto@kyotokagaku.co.jp

Reproducing all or any part of the contents is prohibited without the Kyoto Kagaku's permission.